


Product Information

**(±)-3,4-Methylenedioxymethamphetamine
hydrochloride solution, 1.0 mg/mL±5% in methanol
drug standard**

Catalog Number **M5029**
Lot Number 109K8710
Storage Temperature 2–8 °C

CAS RN: 64057-70-1
42542-10-9 (free base)

Synonyms: MDMA hydrochloride, Ecstasy
hydrochloride, XTC hydrochloride,
5-(N,α-Dimethyl)ethanamine-1,3-benzodioxole
hydrochloride

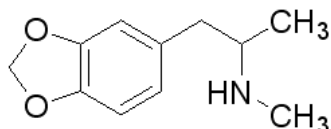

• HCl

Product Description

Molecular Formula: C₁₁H₁₅NO₂ · HCl
Molecular Weight: 229.70

DEA Class: Exempt preparation of Class I

Concentration: 1.17 mg (±)-3,4-methylenedioxy-
methamphetamine hydrochloride (equivalent to 0.984
mg of free base)/mL of GC grade methanol,
concentration verified by UV.

Expiration Date: October 2012

Precautions and Disclaimer


This product is for R&D use only, not for drug,
household, or other uses. Please consult the Material
Safety Data Sheet for information regarding hazards
and safe handling practices.

Storage/Stability

Store the product at 2–8 °C. If stored at 2–8 °C in an
airtight container, protected from light, decomposition of
the product is less than 1% in 36 months. After
opening, concentration may change due to loss of
solvent.


JES, MAM 11/09-1

70 eV Electron Ionization Mass Spectrum

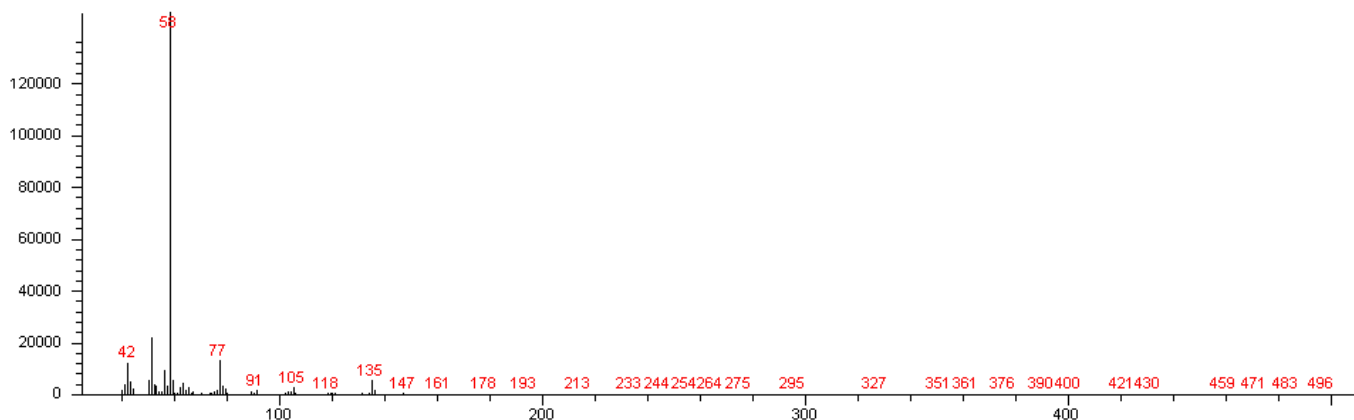

Hewlett-Packard 5890 Series II Gas Chromatograph
Hewlett-Packard 5971 Mass Selective Detector
Hewlett-Packard G1034C MS ChemStation (HP-DOS series)

FT-IR

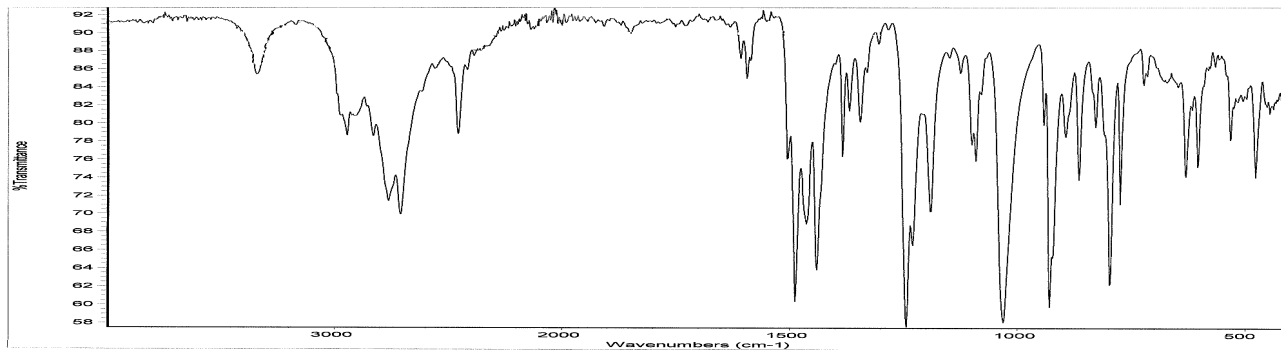


Nicolet 380 FT-IR Thermo Smart Orbit

Ultraviolet Spectrum


Peak	283.0 nm
Absorbance	0.8145
Solvent	0.2 N Sulfuric acid
Dilution	1:24 (v/v)

Capillary Gas Chromatography

Column Supelco SPB-1 (Catalog Number 24162)
I.D. 0.20 mm **Length** 15 m **Film Thickness** 0.20 μm
Oven Temperature 50 °C (2 minutes), then
15 °C/minute to 300 °C, hold 11 minutes
Injector Temperature 250 °C, Split
Detector Hewlett-Packard 5971
Mass Selective Detector (70 eV, 40-500 m/z)

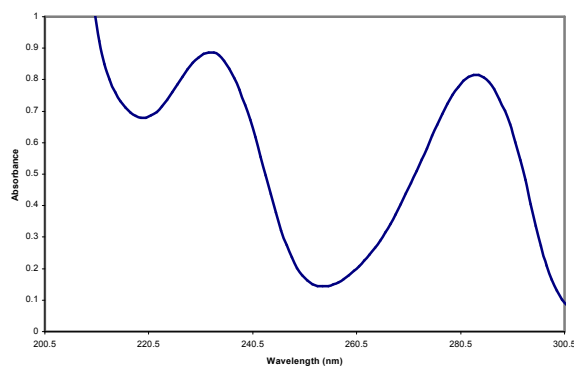

Beckman-Coulter DU 800

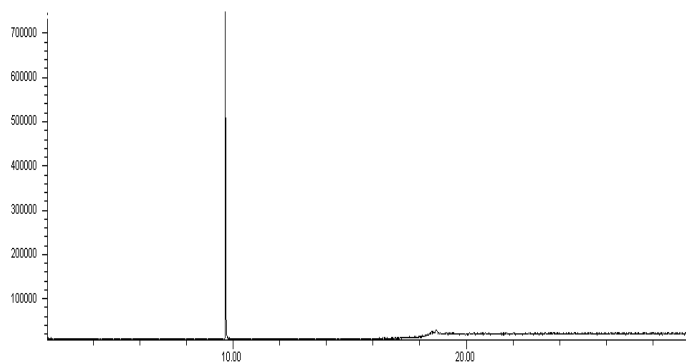

Hewlett-Packard 5890

Sigma brand products are sold through Sigma-Aldrich, Inc.

Sigma-Aldrich, Inc. warrants that its products conform to the information contained in this and other Sigma-Aldrich publications. Purchaser must determine the suitability of the product(s) for their particular use. Additional terms and conditions may apply. Please see reverse side of the invoice or packing slip.