

prepared for PFAS Testing

Fast and High-Resolution LC-MS Separation with Ascentis® Express PFAS HPLC Columns

PFAS (Per- and poly-fluoroalkyl substances) are persistent, man-made organic compounds, widely found in the environment. Recent awareness has brought attention to the toxicity of these substances. The U.S. Food and Drug Administration (FDA) and the U.S. Environmental Protection Agency (EPA) have initiated actions against PFAS. For determination of PFASs, liquid chromatography–mass spectrometry (LC-MS) is a commonly used technique.


The new Ascentis® Express PFAS HPLC column, with its Fused-Core® technology and a particle size of 2.7 µm, delivers fast and high-resolution separations with excellent selectivity, peak shape, and necessary retention to perform in EPA methods 537.1, 533 and 8327.

Key benefits of Ascentis® Express PFAS columns include:

- 2.7 µm Fused-Core® particle for reliable and high efficiency separations and lower column back pressure compared to sub-2 µm particles
- Excellent suitability for MS detection
- Application-related Lot analysis and single column performance testing
- Pressure limit: 600 bar


Ascentis® Express PFAS HPLC columns enable precise MS results

The Ascentis® Express PFAS HPLC column is designed for the separation of novel and legacy short chain and long chain PFAS compounds containing branched and linear isomers, whilst adhering to EPA methodology requirements. Furthermore, a specific PFAS delay column prevents background PFAS contamination from interfering with the sample results in quantitative LC-MS methods.

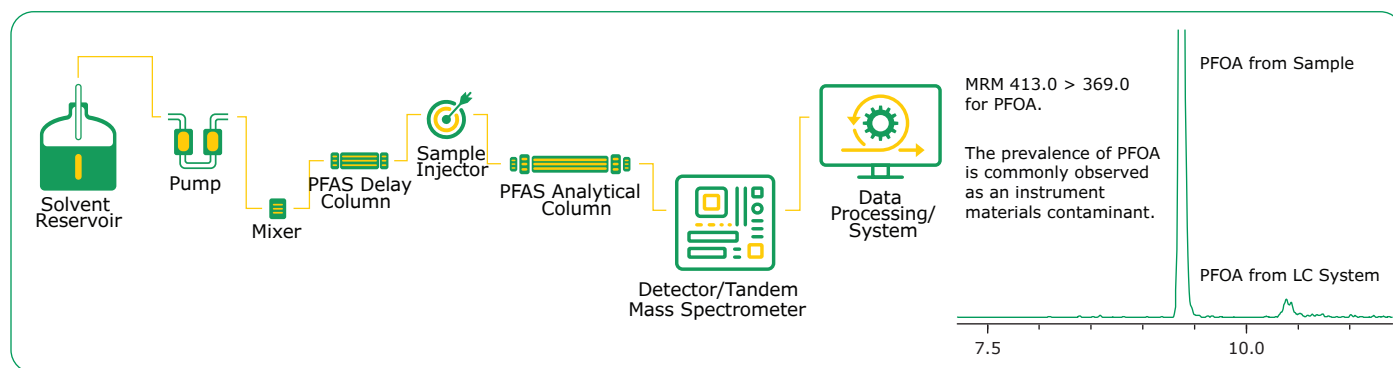

The highly retentive endcapped silane of the Ascentis® Express PFAS Delay column provides high retention of PFAS compounds across various mobile phase conditions and is used to delay background instrument

PFAS contamination from interference with analyzed samples. For this reason, the Ascentis® Express PFAS Delay column is placed upstream of the sample injector and after the mixer.



Analysis of PFAS Compounds in EPA 537.1:

LC Conditions:


Analytical Column	Ascentis® Express PFAS, 2.7 µm, 10 cm x 2.1 mm, 90A
Delay Column	Ascentis® Express PFAS Delay, 2.7 µm, 5 cm x 3 mm
Mobile Phase	A: 10 mM Ammonium Acetate B: Methanol
Flow Rate	0.4 mL/min
Pressure	485 bar
Temperature	35 °C
Injection Volume	2.0 µL
Sample Solvent	Methanol (96%) Water (4%)

Gradient

Time	% B
0.0	33.0
18.0	98.0
18.1	100.0
21.0	100.0
21.1	33.0
26.0	End

MS Condition:

Detection	-ESI MS/MS
ESI LCMS system	Shimadzu LCMS-8040
Spray Voltage	-2.0 kV
Nebulizing gas	2 L/min
Drying gas	15 L/min
DL temp	250 °C
Heat Block	400 °C

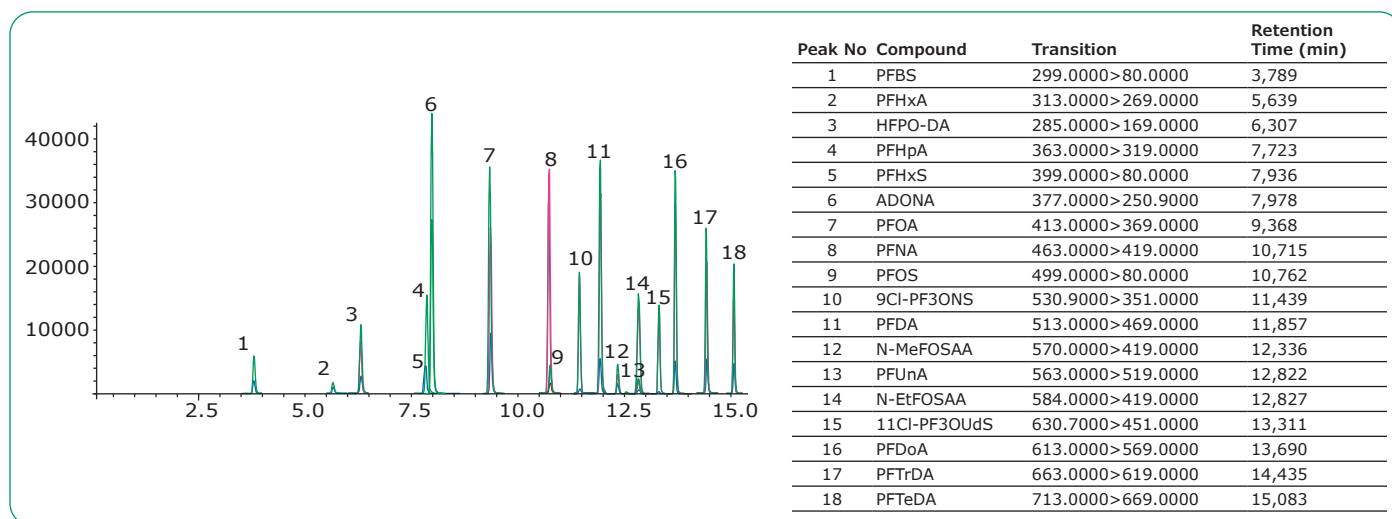

Ordering Information

Ascentis® Express PFAS, 2.7 µm

Length (mm)	ID (mm)	Cat. No.
50 x	2.1	53557-U
100 x	2.1	53559-U
150 x	2.1	53560-U
250 x	2.1	53562-U
50 x	3	53563-U
100 x	3	53564-U
150 x	3	53565-U
250 x	3	53570-U

Ascentis® Express PFAS Delay columns, 2.7 µm

Length (mm)	ID (mm)	Cat. No.
50 x	3	53572-U
50 x	4.6	53573-U

Typically, the delay column is used with a larger ID than the analytical column:

Analytical column	-	Delay Column
2.1 mm ID	-	3 mm ID
3 mm ID	-	4.6 mm ID

To place an order or receive technical assistance


Order/Customer Service: [SigmaAldrich.com/order](https://sigmaaldrich.com/order)

Technical Service: [SigmaAldrich.com/techservice](https://sigmaaldrich.com/techservice)

Safety-related Information: [SigmaAldrich.com/safetycenter](https://sigmaaldrich.com/safetycenter)

Merck KGaA
Frankfurter Strasse 250
64293 Darmstadt, Germany

[SigmaAldrich.com](https://sigmaaldrich.com)




PFAS analysis requires precision at every step.

MilliporeSigma has products specifically developed to support PFAS analysis including:

- Supelco® HPLC Columns
- Millipore® PFAS-free Membrane Filters
- Supelco® Sample Prep Solutions
- Supelco® Reference Materials
- Sigma-Aldrich® Solvents for PFAS Analysis
- Milli-Q® Lab Water Solutions
- PFAS-free labware through our partnerships with brands you know and trust

Be confident in your results with our trusted products and services for your entire workflow.

Perfect your PFAS protocol
SigmaAldrich.com/PFAS

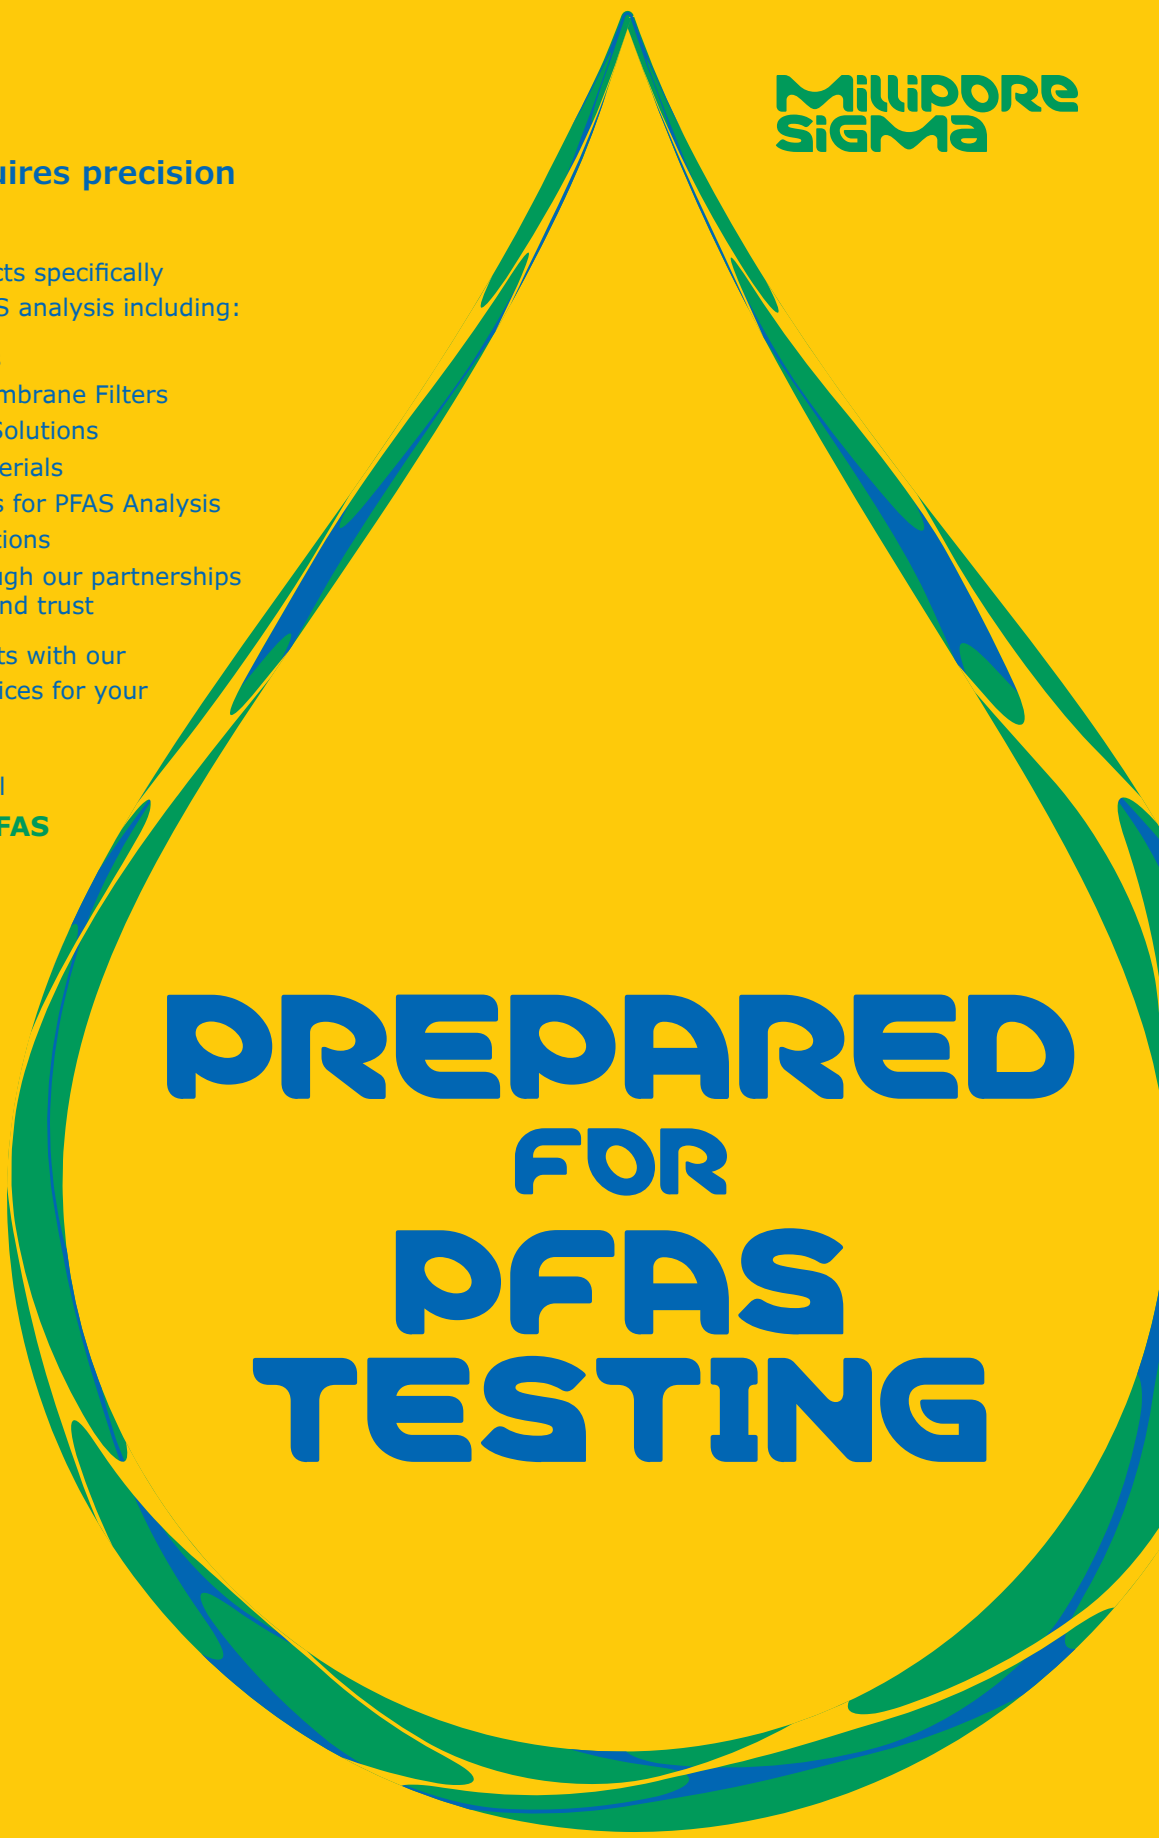A large, stylized water drop graphic that serves as a background for the central text. The drop is outlined in blue and filled with a gradient of green and blue, with some internal blue streaks. The text "PREPARED FOR PFAS TESTING" is centered within the drop in a bold, blue, sans-serif font.

PREPARED FOR PFAS TESTING

The life science business of Merck KGaA, Darmstadt, Germany operates as MilliporeSigma in the U.S. and Canada.

© 2021 Merck KGaA, Darmstadt, Germany and/or its affiliates. All Rights Reserved. MilliporeSigma and the vibrant M are trademarks of Merck KGaA, Darmstadt, Germany or its affiliates. All other trademarks are the property of their respective owners. Detailed information on trademarks is available via publicly accessible resources.



Sigma-Aldrich®
Lab & Production Materials

Millipore®
Preparation, Separation,
Filtration & Monitoring Products

Supelco®
Analytical Products

Milli-Q®
Lab Water Solutions