

Product Information


**Buprenorphine hydrochloride solution,
1.0 mg/mL±5% in methanol
drug standard**

Catalog Number **B7536**
Lot Number 058K8708
Storage Temperature -20 °C

CAS RN 53152-21-9
Synonyms: 21-Cyclopropyl-7α-[(S)-1-hydroxy-
1,2,2-trimethylpropyl]-6,14-indo-ethano-
6,7,8,14-tetrahydrooripavine hydrochloride

Product Description

Molecular Formula: C₂₉H₄₁NO₄ · HCl
Molecular Weight: 504.10

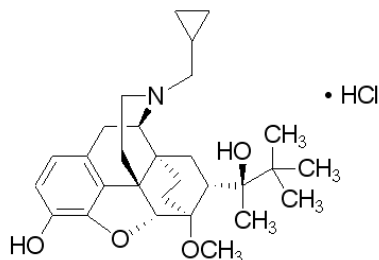

Concentration: 1.08 mg of Buprenorphine hydrochloride
(equivalent to 1.00 mg of free base)/mL of GC grade
methanol, concentration verified by UV.

Expiration Date: April 2012

Precautions and Disclaimer

This product is for R&D use only, not for drug,
household, or other uses. Please consult the Material
Safety Data Sheet for information regarding hazards
and safe handling practices.


Storage/Stability

Store the product at -20 °C. If stored at -20 °C in an
airtight container, protected from light, decomposition of
the product is less than 2% in 12 months. After
opening, concentration may change due to loss of
solvent.

DEA Class: Exempt preparation of Class III


CMW,MAM 04/08-1

70 eV Electron Ionization Mass Spectrum

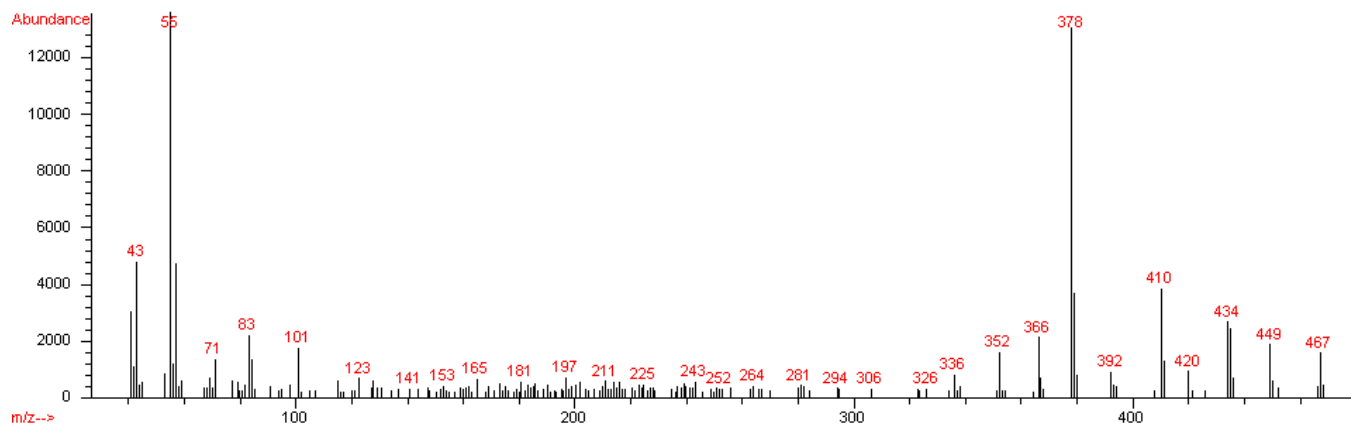

Hewlett-Packard 5890 Series II Gas Chromatograph
Hewlett-Packard 5971 Mass Selective Detector
Hewlett-Packard G1034C MS ChemStation (HP-DOS series)


FT-IR

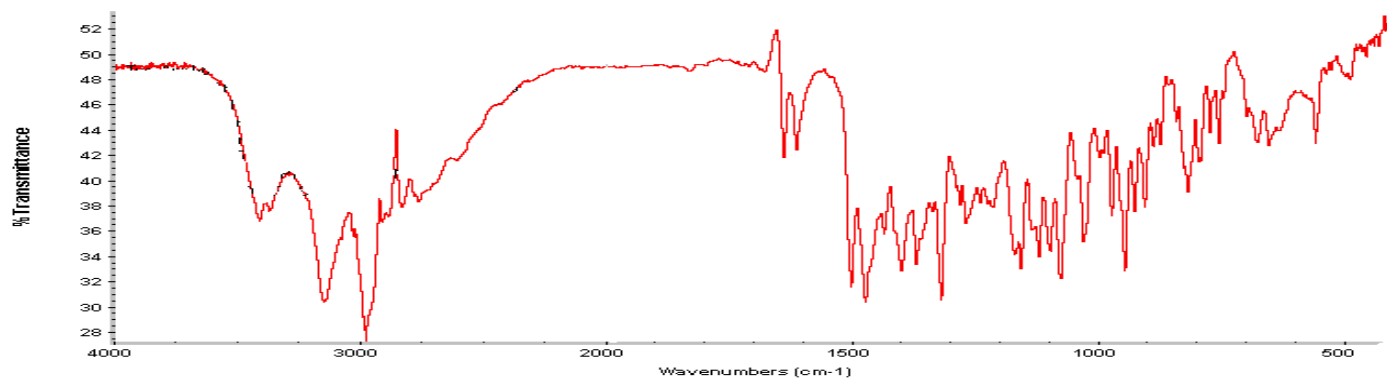

Nicolet Magna IR Spectrometer Series II

Ultraviolet Spectrum


Peak	285.5 nm
Absorbance	0.7360
Solvent	0.2 N H ₂ SO ₄
Dilution	1:4 (v/v)

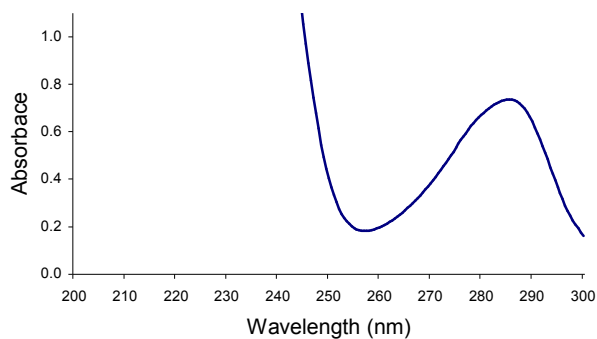

Beckman-Coulter DU 800

Capillary Gas Chromatography

Column Supelco SPB-1 (Catalog Number 24162)
I.D. 0.20 mm **Length** 15 m **Film Thickness** 0.20 µm
Oven Temperature 50 °C (2 minutes), then
15 °C/minute to 300 °C, hold 11 minutes
Injector Temperature 250 °C, Split
Detector Hewlett-Packard 5971
Mass Selective Detector (70 eV, 40-500 m/z)

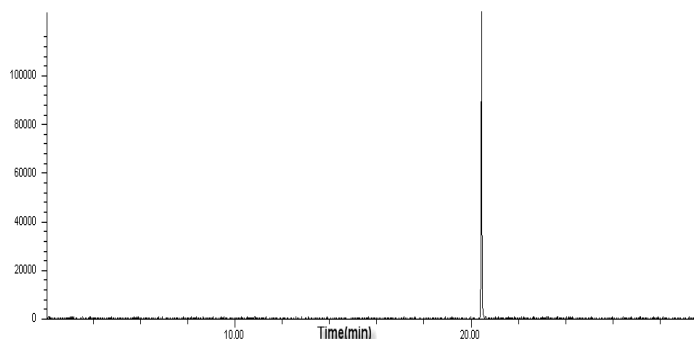

Hewlett-Packard 5890

Sigma brand products are sold through Sigma-Aldrich, Inc.

Sigma-Aldrich, Inc. warrants that its products conform to the information contained in this and other Sigma-Aldrich publications. Purchaser must determine the suitability of the product(s) for their particular use. Additional terms and conditions may apply. Please see reverse side of the invoice or packing slip.